

Radiation Polymerization

Radiation Bioengineering

Radiation Bioengineering

Use made of radiation-induced polymerization, crosslinking and grafting reactions, to produce

- Biocompatible materials**
- Immobilized bioactive materials**

Biocompatible Materials

- **Biological systems (e.g. humans) react adversely to many synthetic polymers**
 - **Important to modify polymer surfaces to make them biocompatible**
- **Thromboresistant materials (blood-compatible materials) have been successfully made, e.g., by**
 - **Radiation-grafting of N,N-dimethylacrylamide onto Aflon (polytetraethylene and ethylene-tetrafluoroethylene copolymers)**
 - **Radiation-grafting of N-vinyl-2-pyrrolidone onto silicone or polyethylene tubes**

Woods and Pikaev (1994)

Biocompatible Products

- **Soft contact lenses**
 - Crosslinked hydrogels by radiation polymerization of 2-hydroxyethyl methacrylate + ethylene glycol dimethacrylate
 - Grafting of N-vinyl-pyrrolidone onto silicone rubber
- **Contact lenses**
 - Low temperature ($\sim -80^{\circ}\text{C}$) radiation polymerization of 2-hydroxymethyl methacrylate (radiation casting)
 - Other plastic lenses also made by radiation casting
- **Heat-shrinkable connectors for severed blood vessels**
 - Radiation crosslinking of trans-1,4-polyisoprene (electron irradiation in air, 100-200 kGy at 300 kGy/h)

Woods and Pikaev (1994)

Immobilized Bioactive Materials

- **Benefits of immobilization**
 - **Controlled slow release of biologically active components, e.g., drugs**
 - **Anchoring the bioactive component for repeated use, e.g., enzymes**
 - **Shaping the material to a desired form, e.g., artificial organs, blood-compatible surfaces**
- **Two widely used methods for immobilization**
 - **Chemical bonding of bioactive material and a benign inactive support**
 - **Trapping bioactive material in a polymer matrix**


Immobilized Bioactive Materials

- Many applications, the most well known being slow-release drugs

Immobilized Species	Applications
Enzymes	Artificial organs, bioreactors, biosensors, separations, therapeutic agents
Antibodies and antigens	Biosensors, diagnostics, drug-delivery systems, immunoassays, separations
Antithrombogenic agents	Blood-compatible surfaces
Drugs	Drug-delivery systems, drug mechanism studies
Neurotransmitters, hormones	Biosensors
Cells and organelles	Artificial organs, bioreactors, biosensors

Woods and Pikaev (1994)


Immobilization of Bioactive Materials

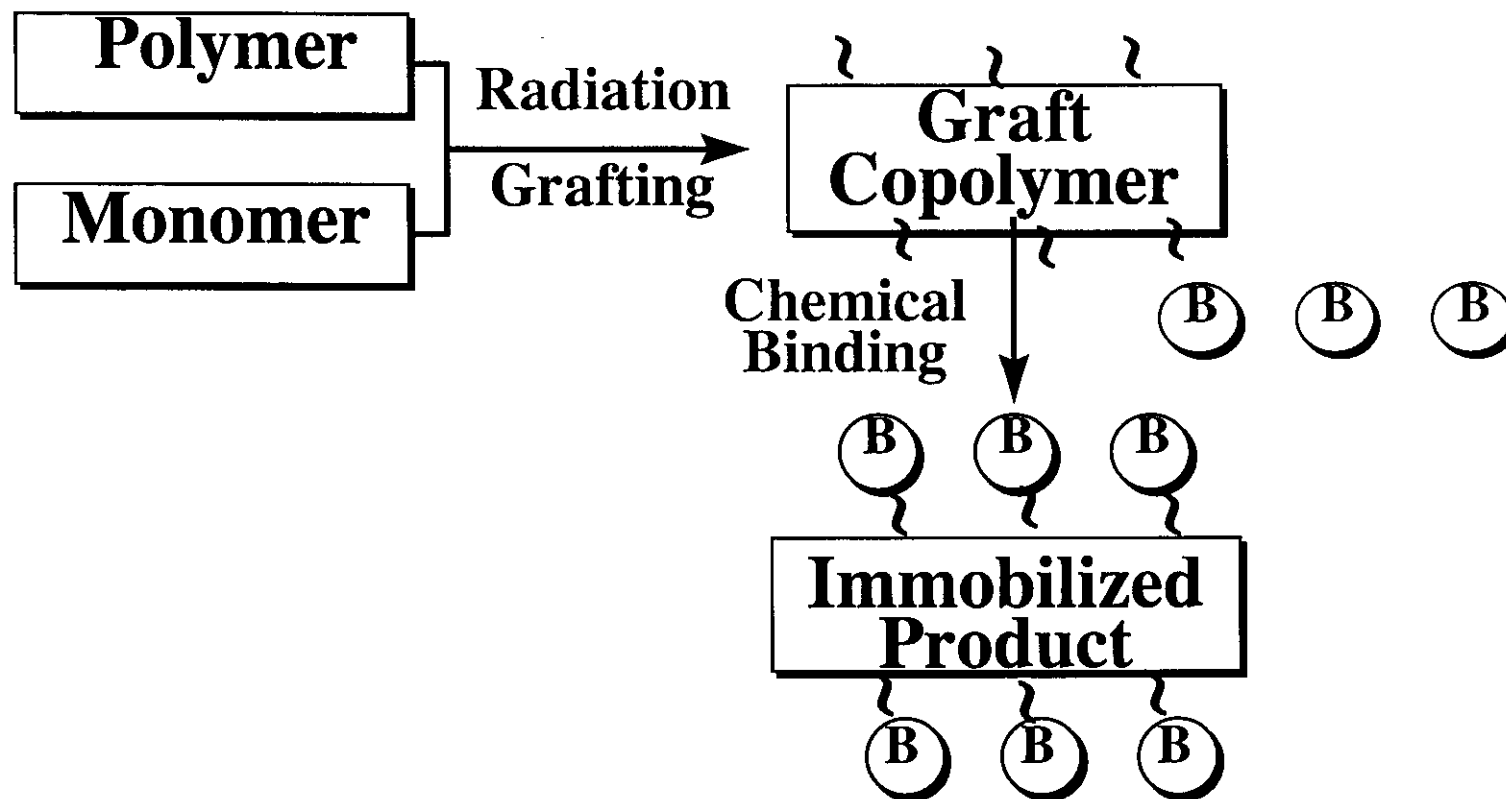


- Immobilization of a bioactive component by chemical bonding to a graft copolymer formed by irradiation

Immobilization of Bioactive Materials

- **Entrapment**

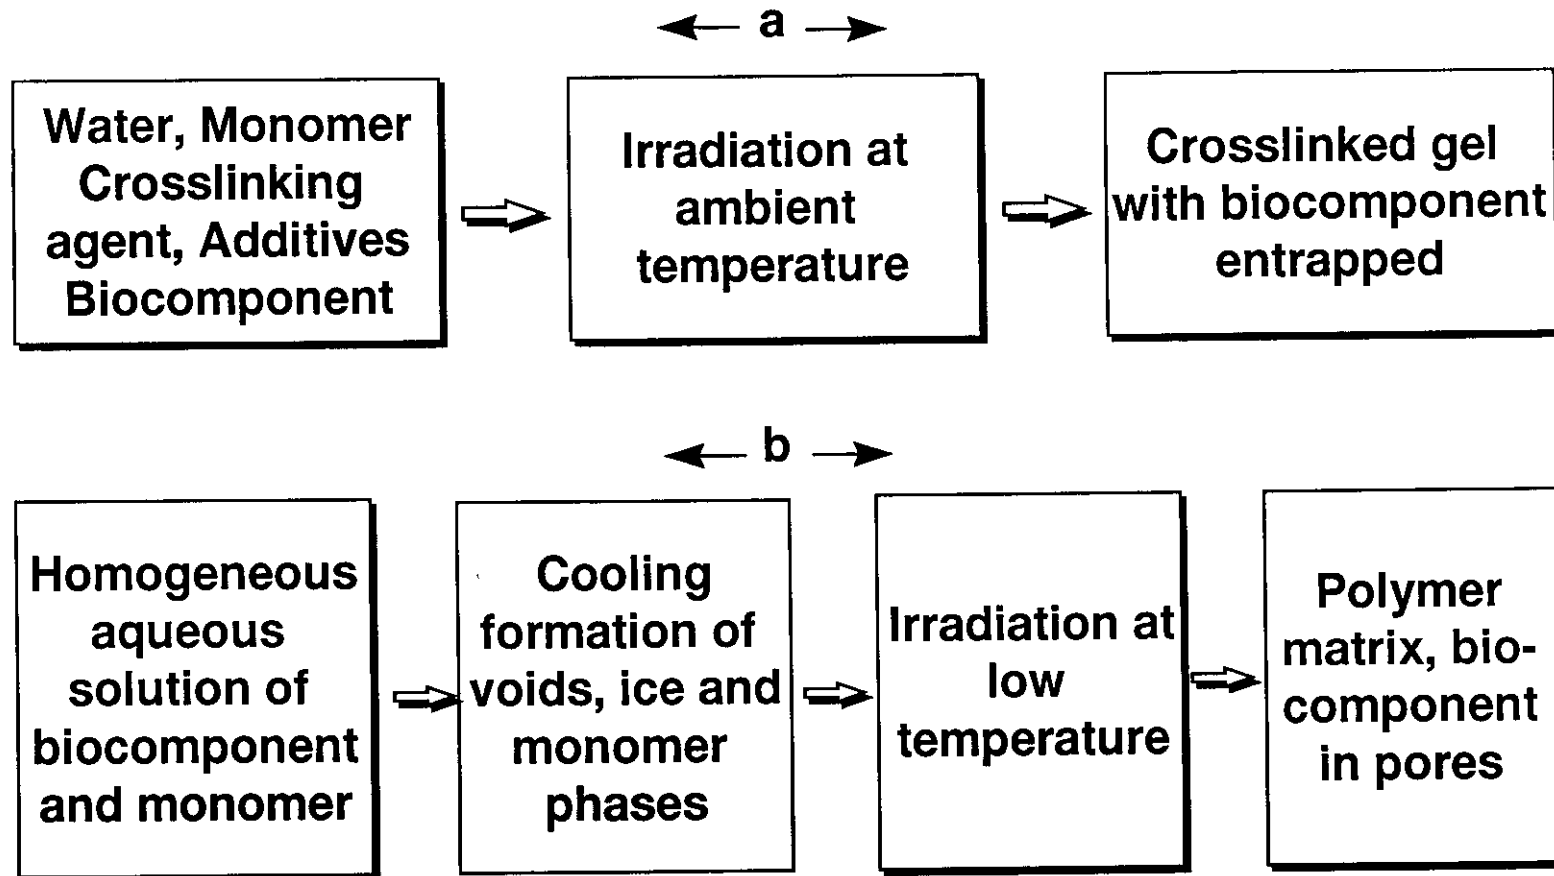


Variation of Drug Release Rate With Hydrophilicity and Molecular Weight

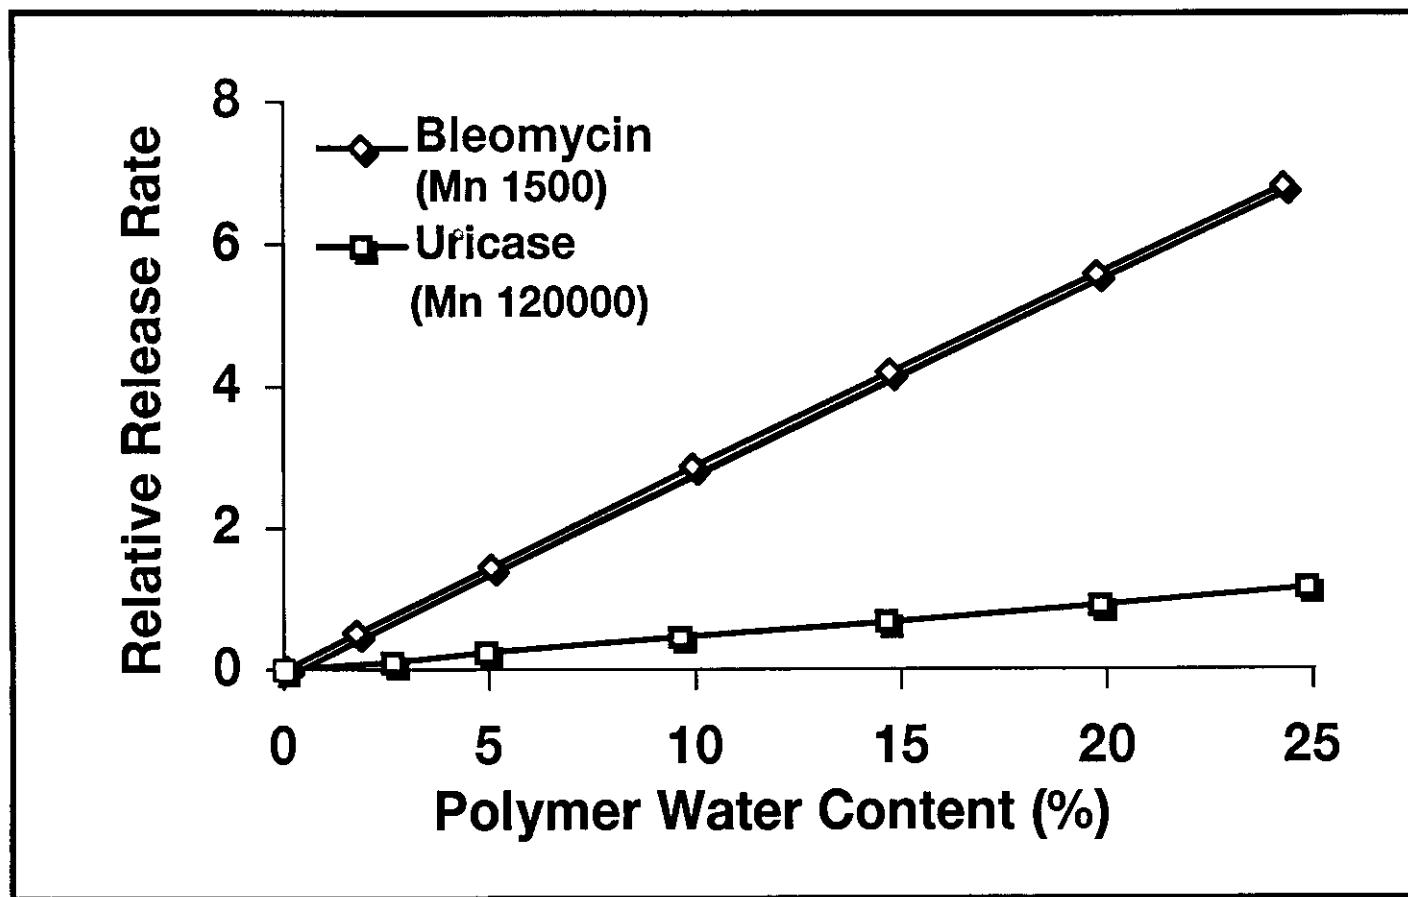


Variation of Drug Release Rate With Hydrophilicity and Molecular Weight (contd)

- **Gamma-radiation-induced polymerization of monomers containing drugs at -78 °C**
- **Hydrophilicity changed by choosing polymers of different contents (2-hydroxyethyl methacrylate, ethylene glycol dimethacrylate, hydroxypropyl acrylate, tetraethylene glycol dimethacrylate, diethylene glycol dimethacrylate, and trimethylpropane triacrylate**
- **Release rates measured at 32°C**

Variation of Release Rates of a Hormone at 32°C With Type of Polymer Entrapment (Kaetsu, 1992)

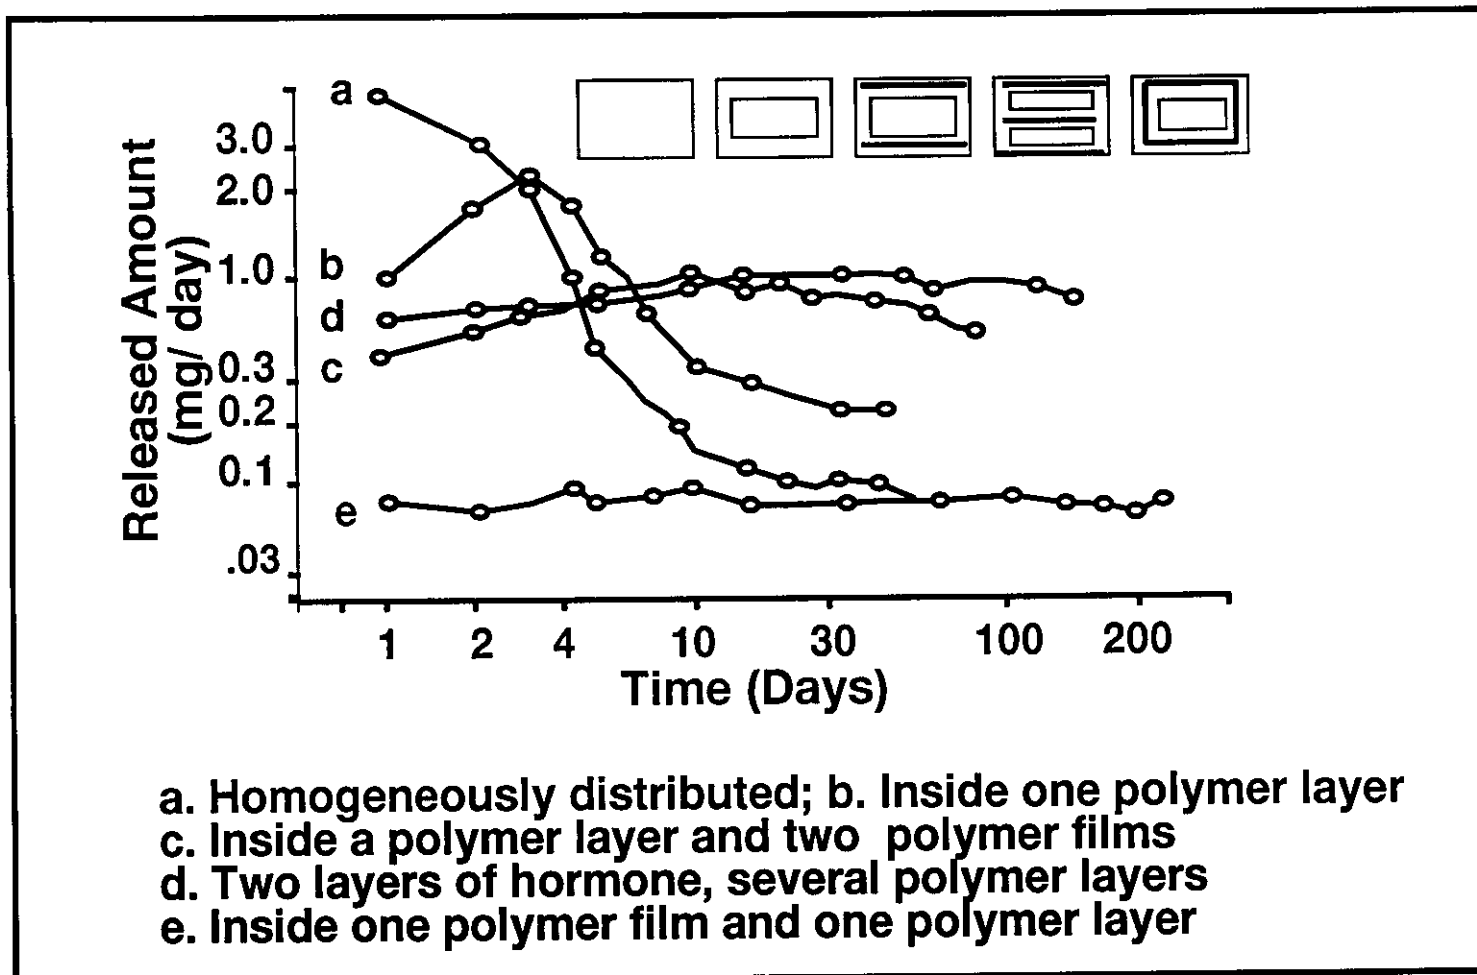


The Insulin Pump



G:Glucose → **GI:Gluconic Acid** → **NR₂:Aminoic Group**
I:Insulin

☼:Glucoseoxidase



-NR₂H⁺ groups
expand membrane
allowing I to migrate
from c to a and b

Release of
Insulin

pH equilibration restores
membrane structure in b,
stopping migration of I

Enzyme Immobilization

- **L-Aspartamine, an enzyme**
 - **Used to treat lymphatic leukemia**
 - **Shows undesirable side effects**
 - **Immobilized product better**
- **Steps in immobilization**
 - **Radiation grafting of methacrylic acid onto polypropylene, PP-COOH**
 - **Treatment with carbodiimide to give acylisourea derivative**
 - **Treatment with N-hydroxysuccinimide**
 - **Reaction with the enzyme**



- **Has also been immobilized on cellulose**

Woods and Pikaev (1994)

Tissue - Compatible Materials

- **Skin covering**
 - **Radiation crosslinked polyacrylamide and polyvinyl pyrrolidone used as wound dressing**
 - **Radiation grafted cotton gauge/acrylamide/provital; used as burn dressing which releases provital slowly**
- **Ocular disks/contact lenses**
 - **Radiation polymerized disks from a solution of N-vinylpyrrolidone, 2-hydroxyethyl methacrylate and pilocarpin hydrochloride, used to treat glaucoma**

Kaetsu (1992); Woods and Pikaev (1994)

Conclusions

- **The use of radiation processing in the bioengineering field would continue to increase**
- **An important advantage of radiation processing in immobilization of bioactive materials is that the substrates are not exposed to high temperatures; most bioactive materials are heat-sensitive**